

6001067

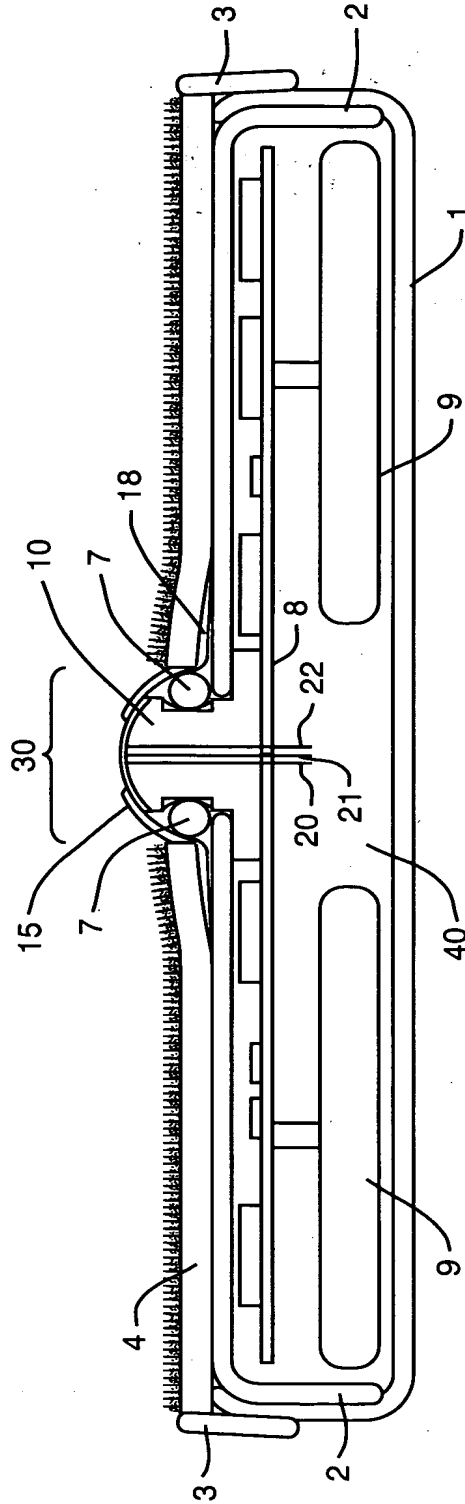


FIG. 1A

2013
NOV 15 10
U.S. PAT. & TM. OFF.

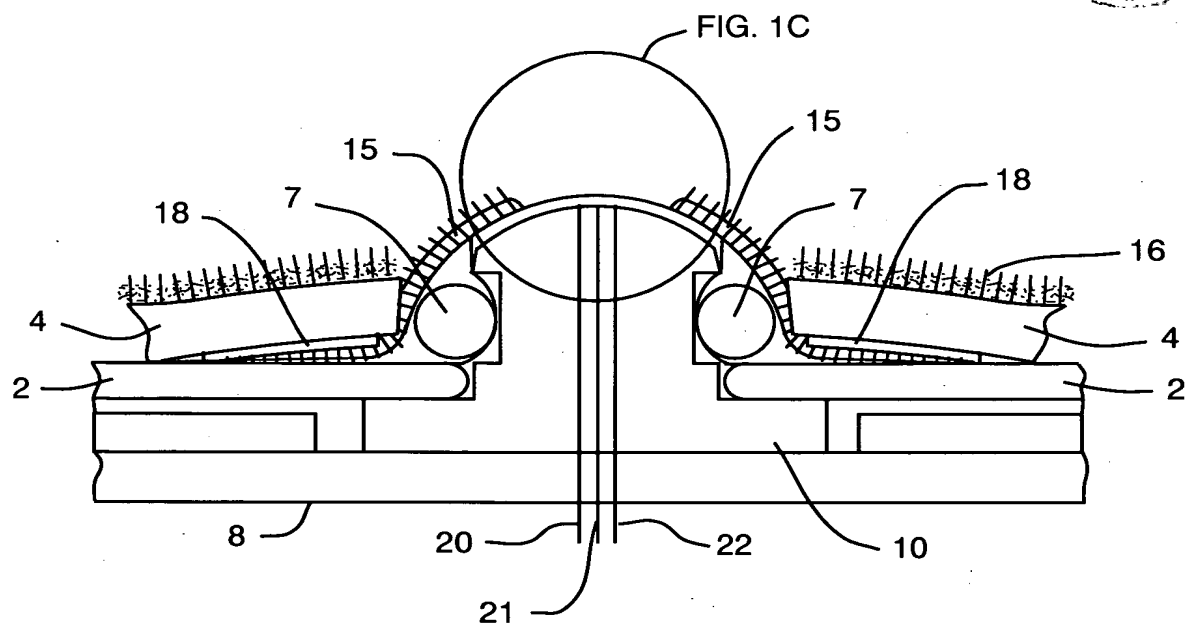


FIG. 1B

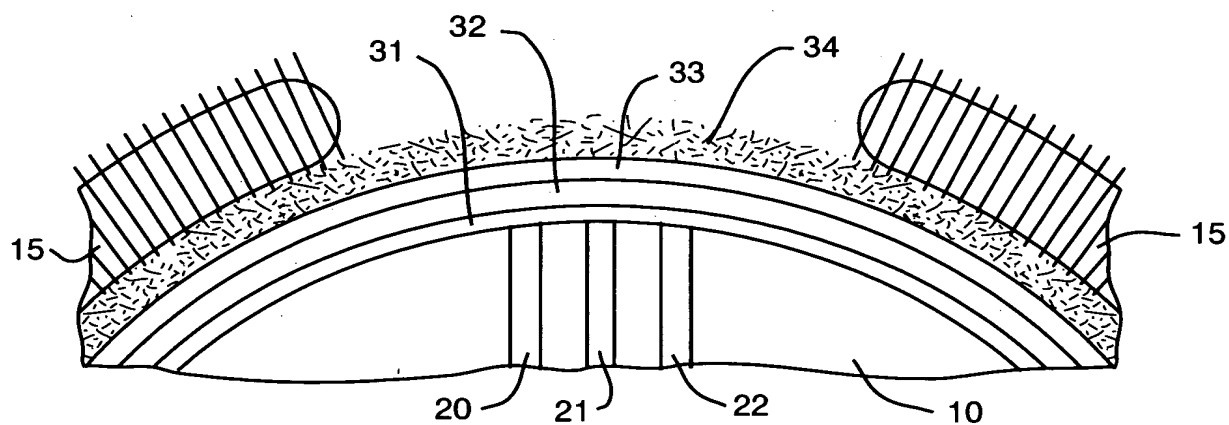


FIG. 1C


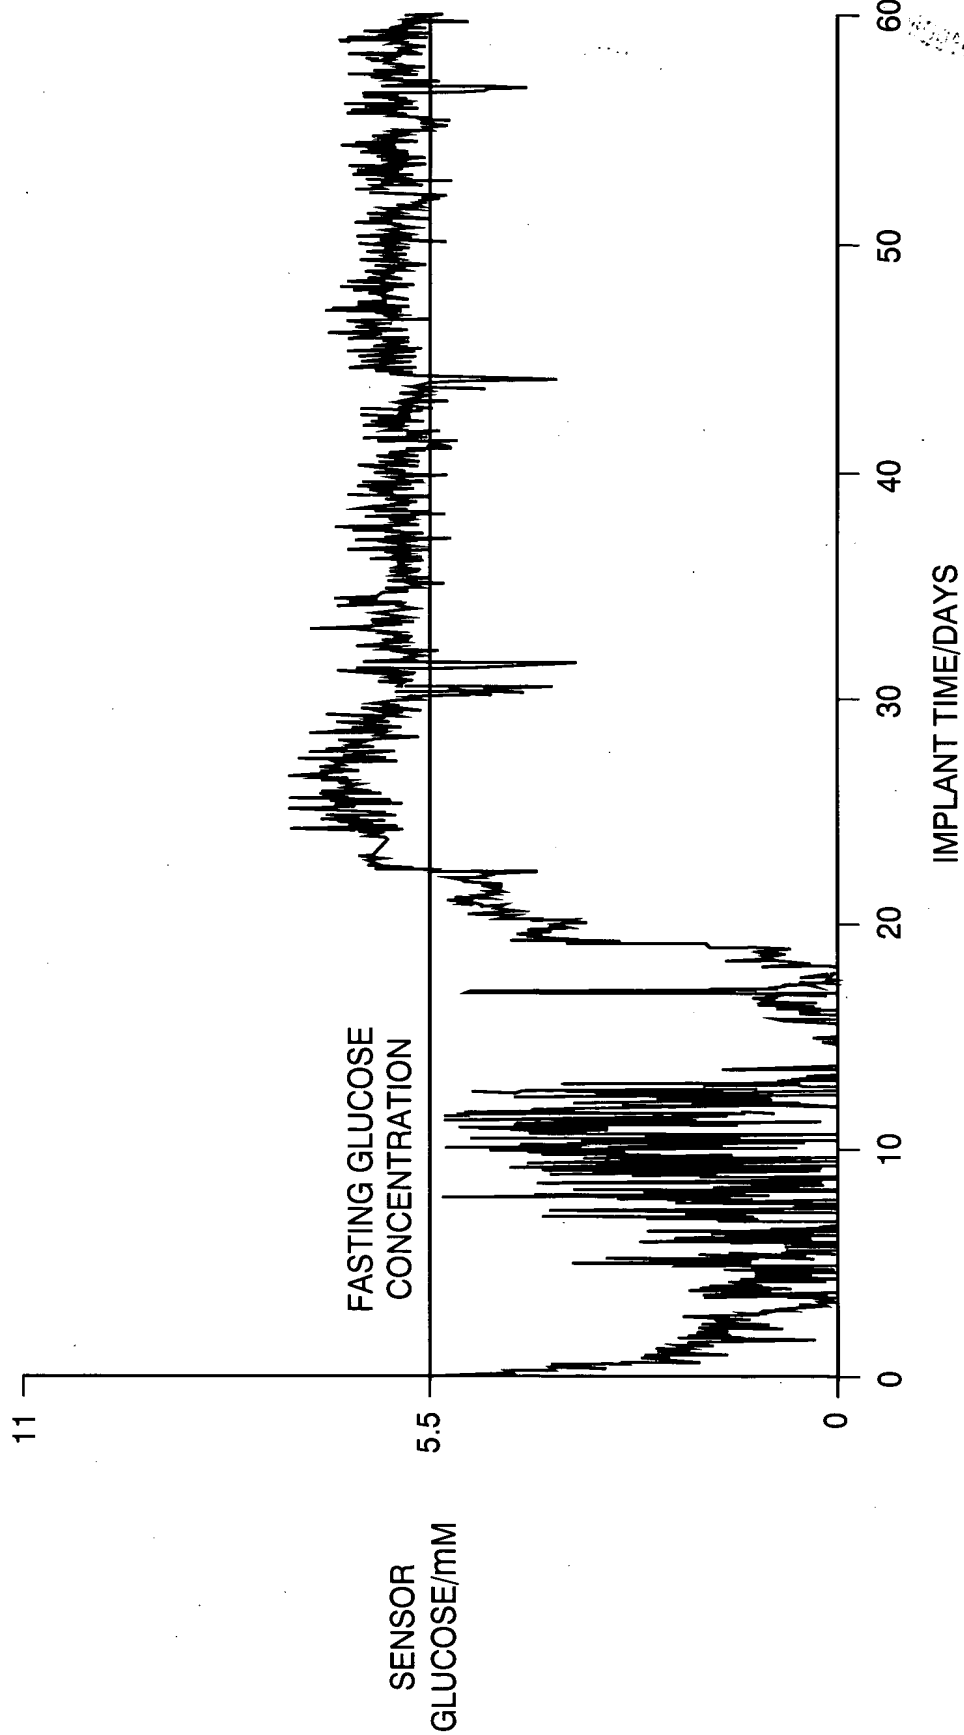


FIG. 2



SENSOR
GLUCOSE/
(mg/dl)

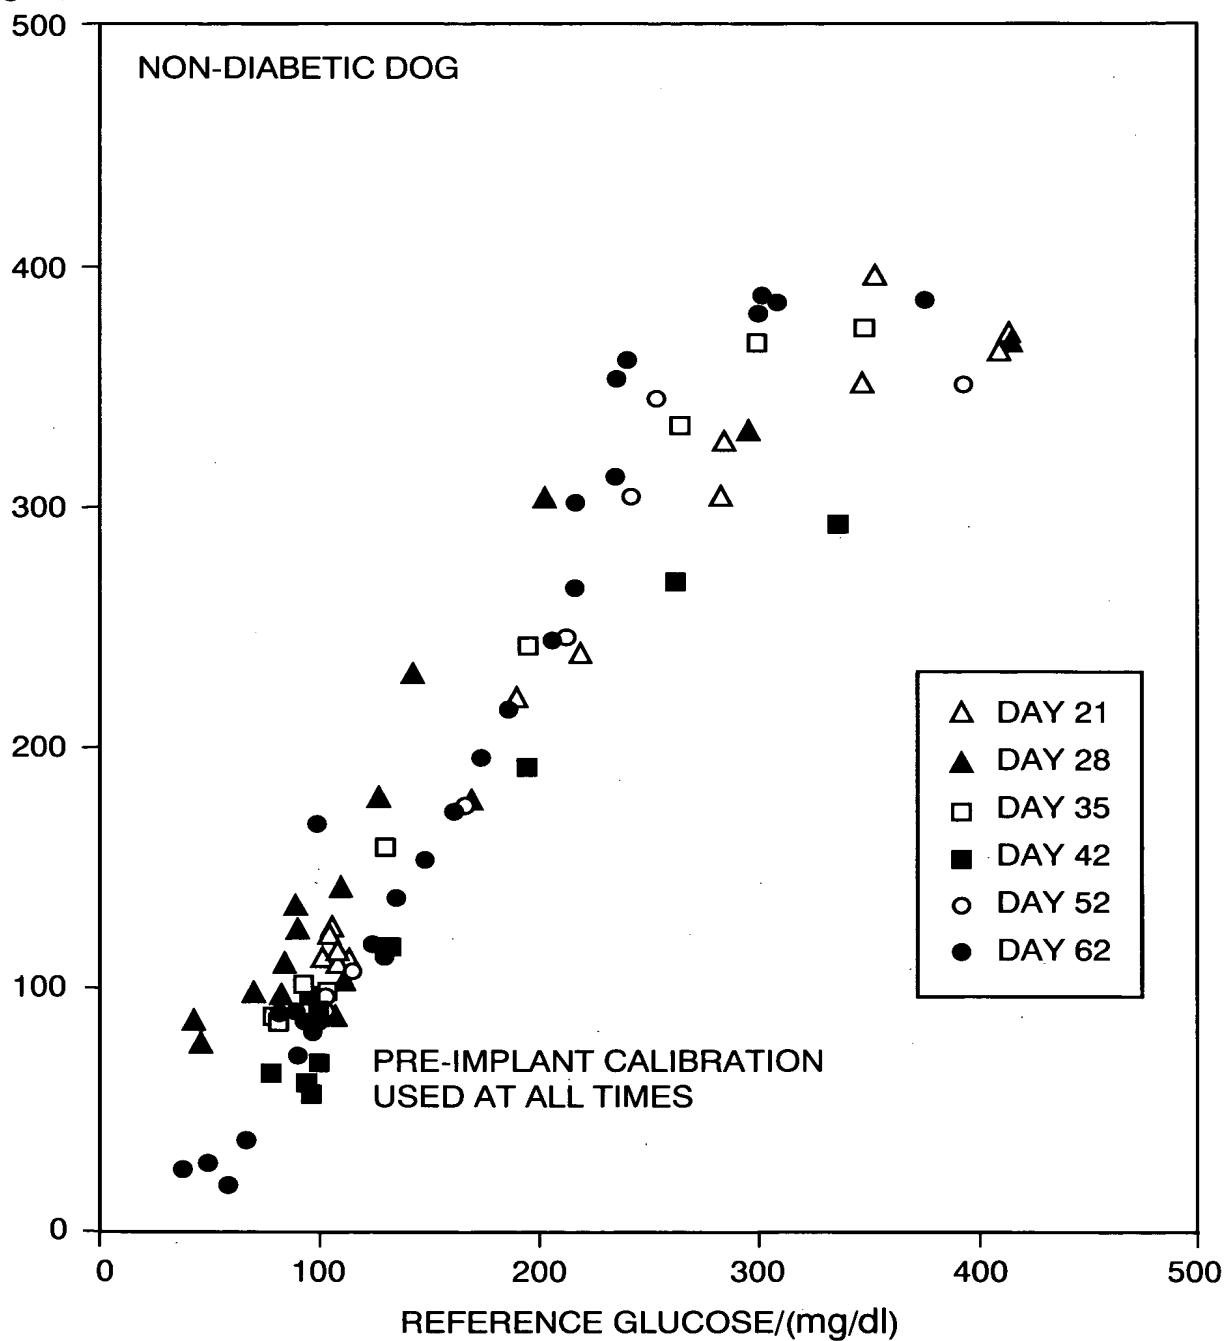


FIG. 3

CURRENT/(nA)

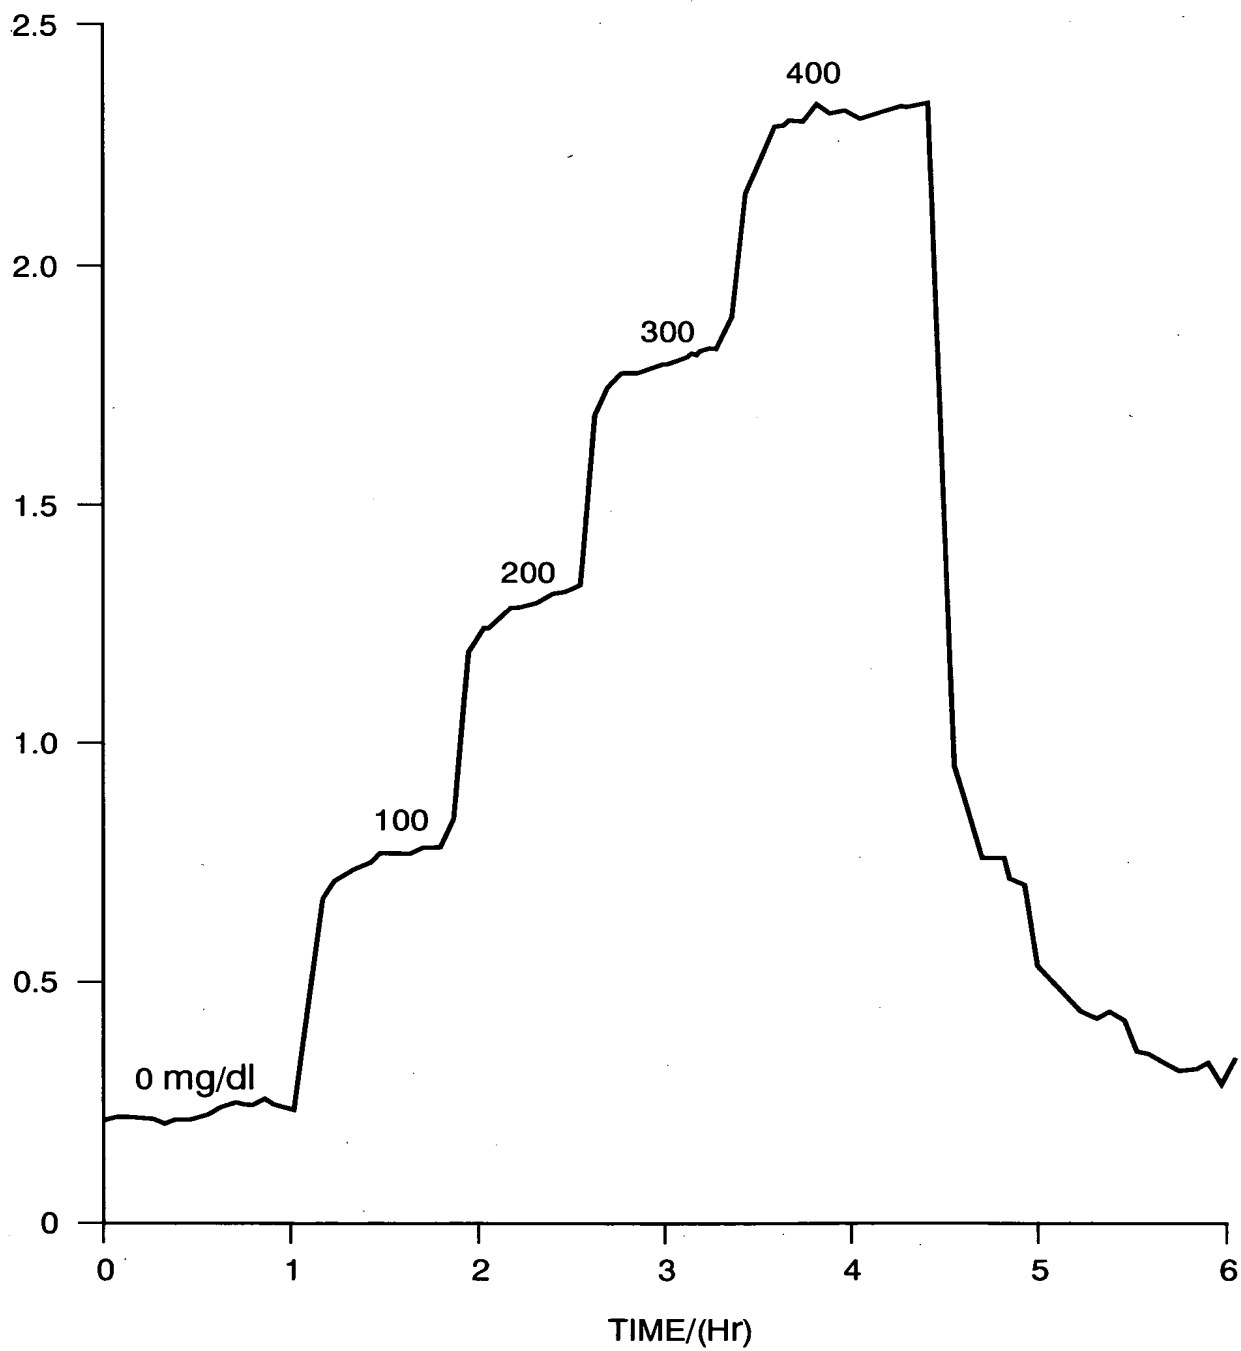


FIG. 4

GLUCOSE
CONCENTRATION/
(mg/dl)

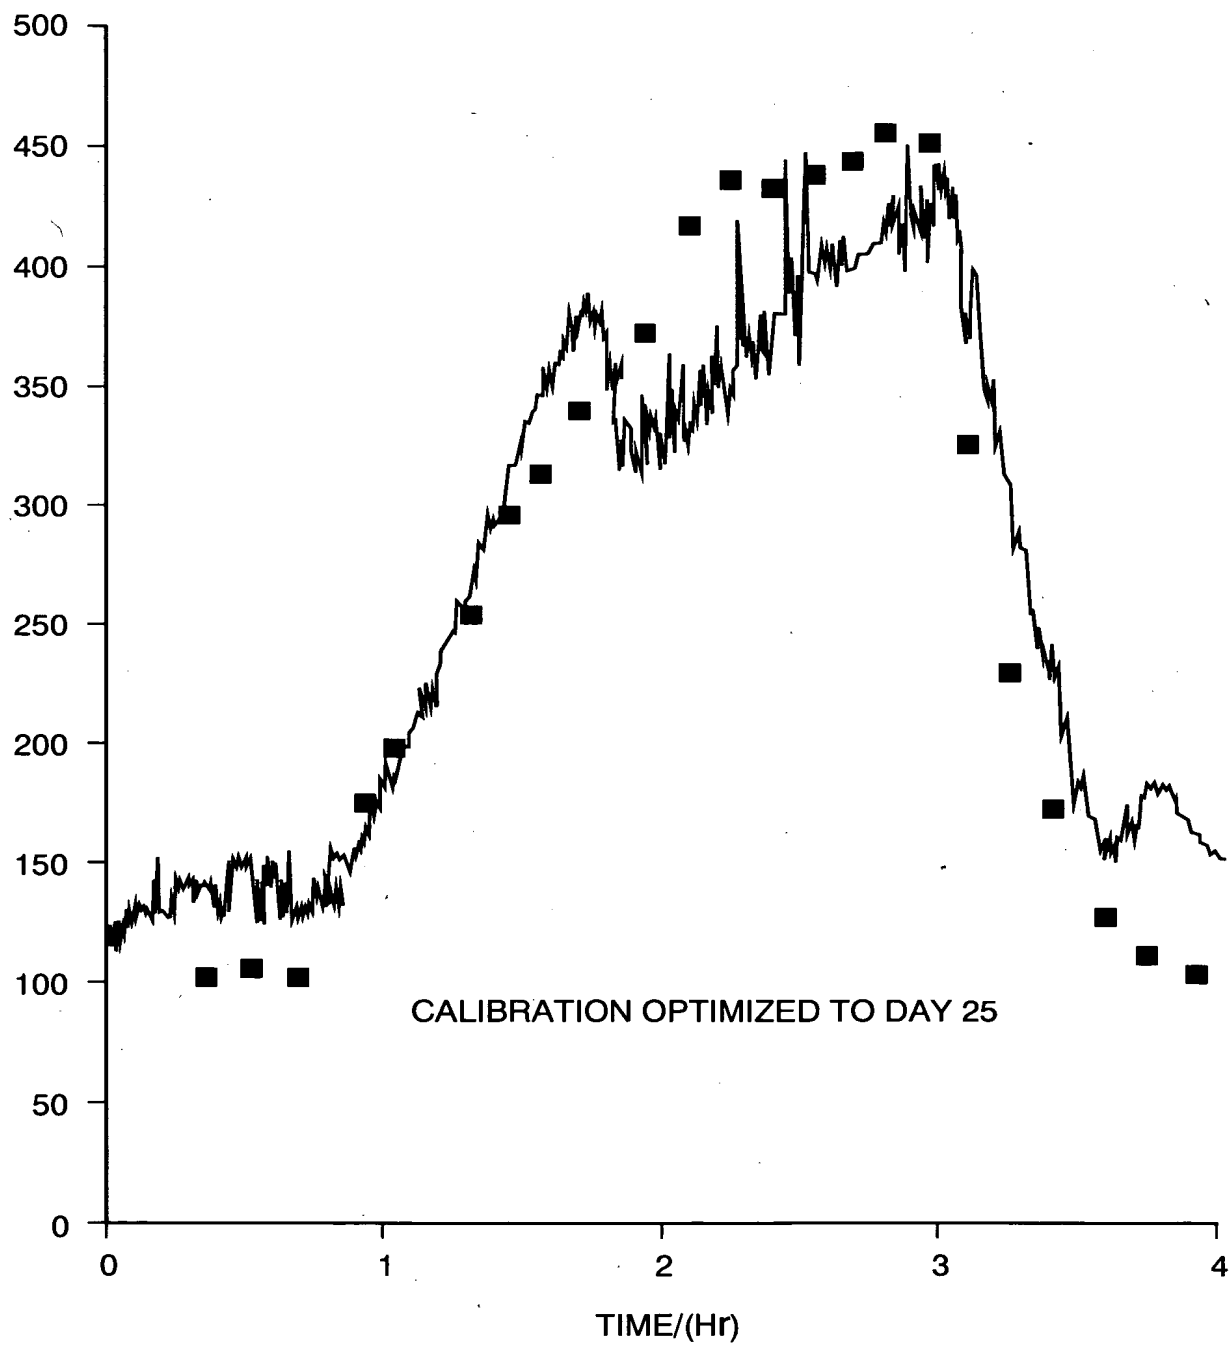


FIG. 5A

GLUCOSE
CONCENTRATION/
(mg/dl)

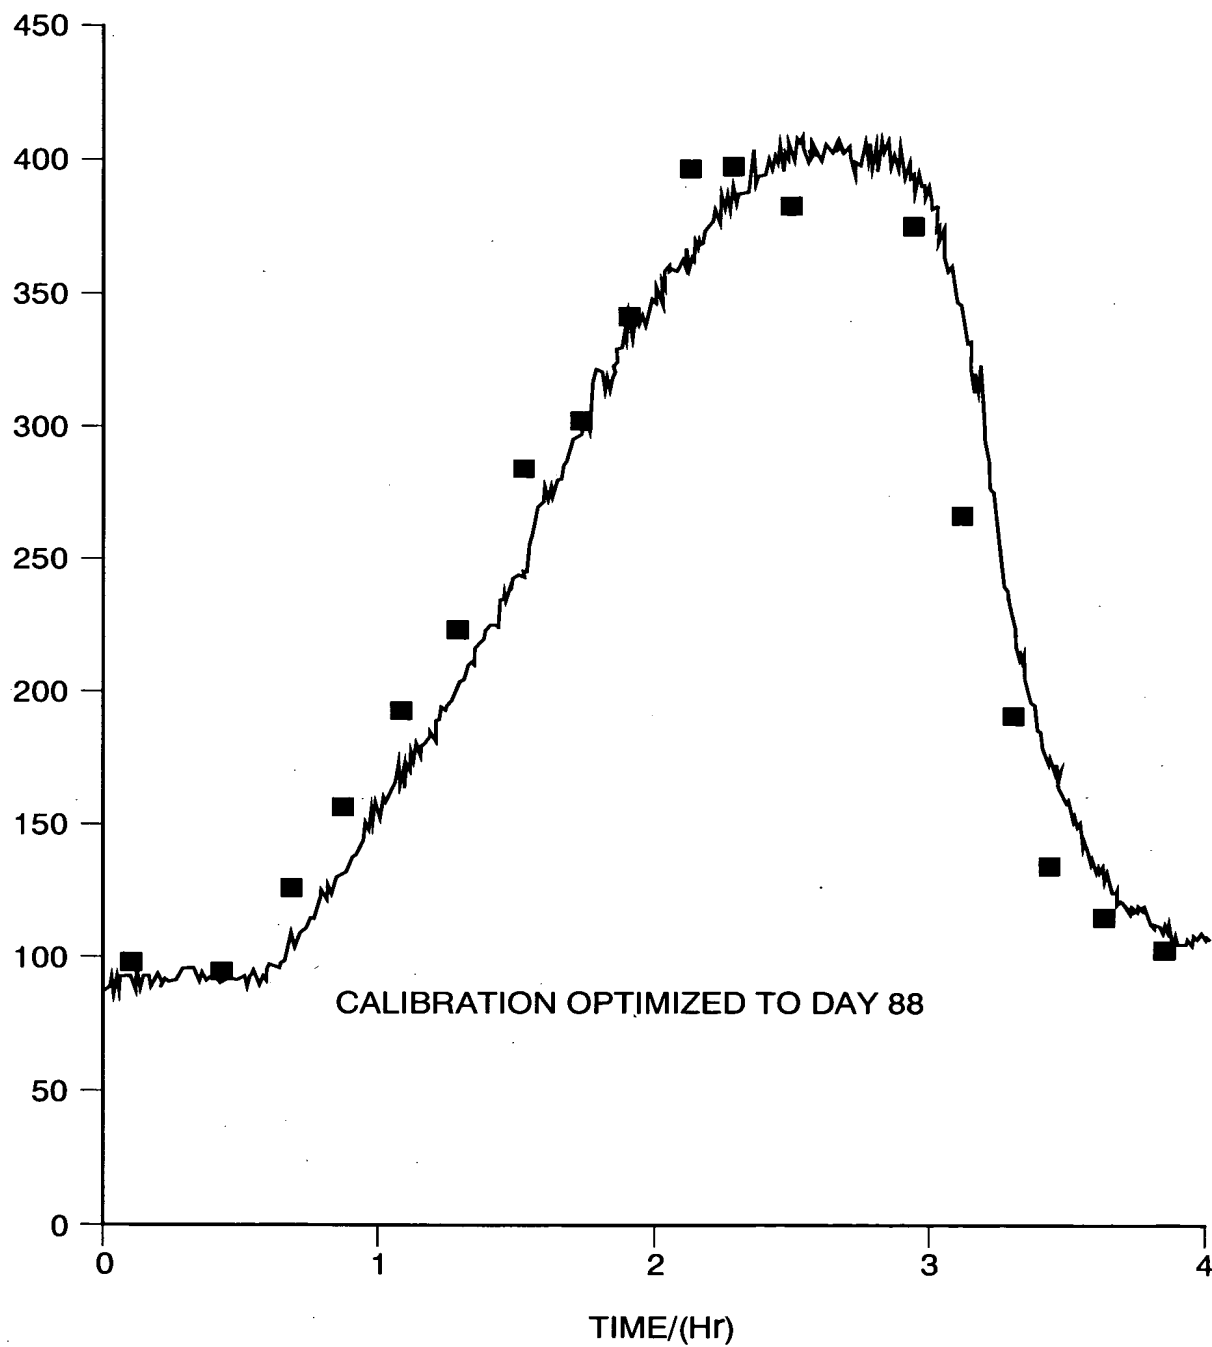


FIG. 5B

GLUCOSE
CONCENTRATION/
(mg/dl)

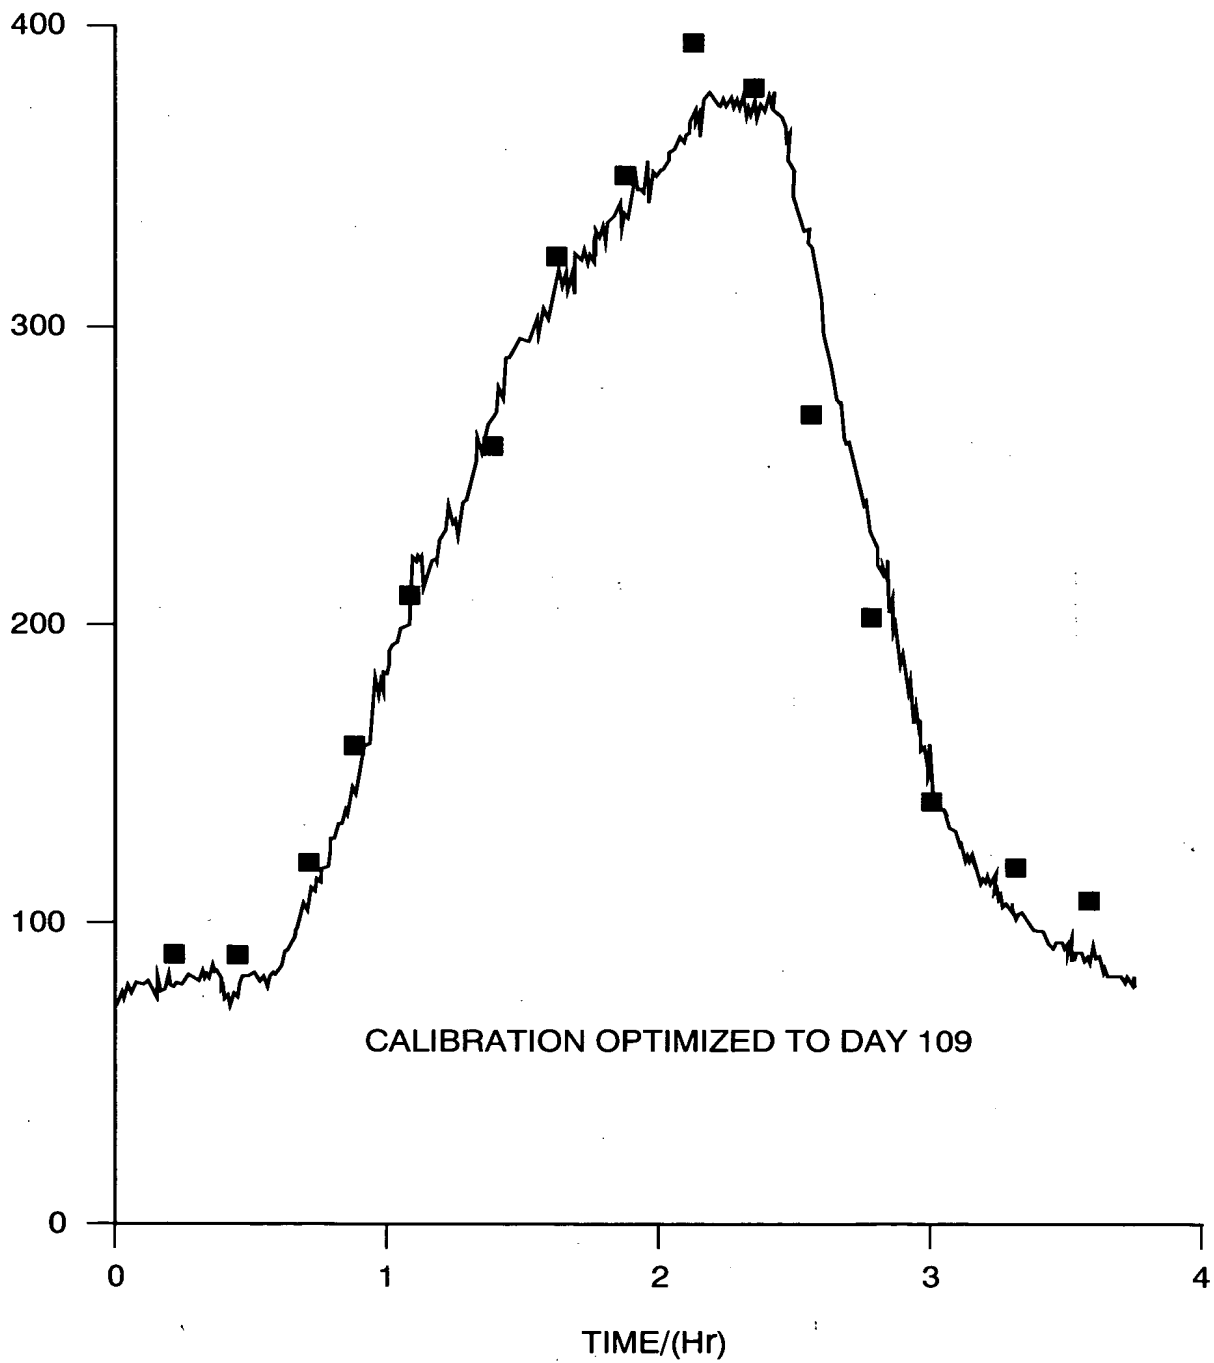


FIG. 5C

SENSOR
GLUCOSE/
(mg/dl)

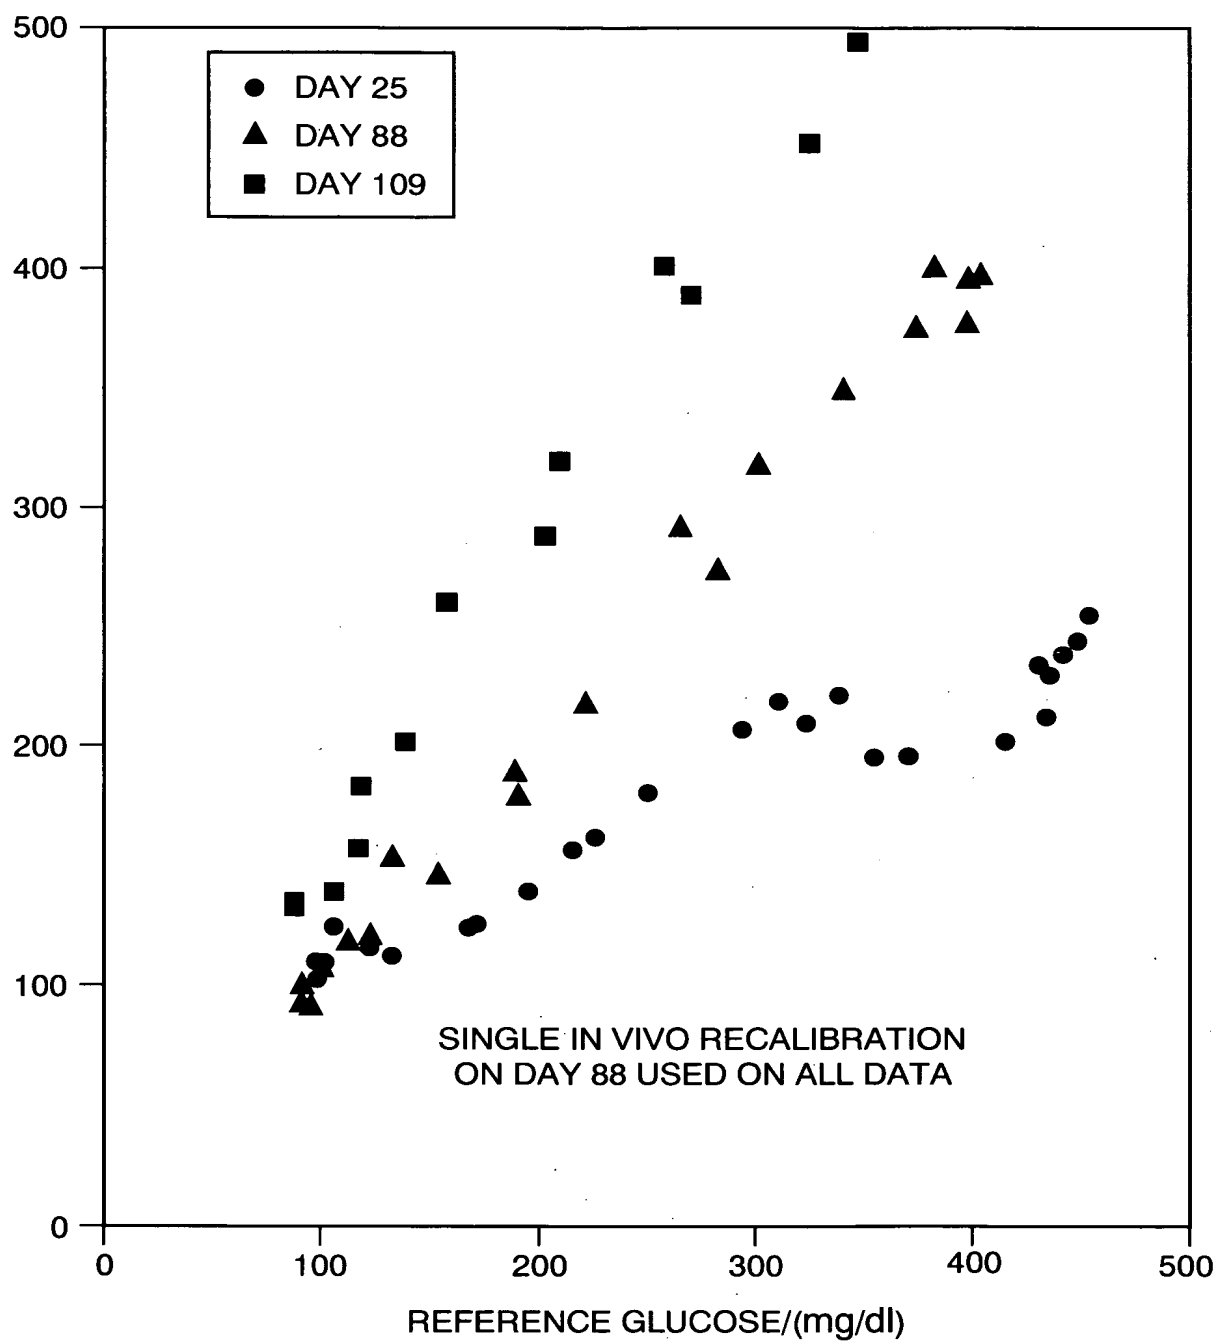


FIG. 6